



A WATTS Brand

175

Medicine Cabinet

## Model 175 — Recessed **BradEX**®

### Model 175-10 — Semi-Recessed

(recesses 2"; projects 2<sup>13</sup>/<sub>32</sub>" )

### Model 175-11 — Surface-Mounted

(projects 4<sup>13</sup>/<sub>32</sub>" )

- ☒ Full Size Mirror
- ☒ Reversible in the Field

## Product Materials

**FLANGE:** 22 gauge stainless steel with exposed surfaces in architectural satin finish. One-piece seamless construction, 1" wide with ¼" return.

**CABINET:** 26 gauge stainless steel.

**DOOR:** 22 gauge stainless steel with heavy-duty full-length piano hinge. Equipped with magnetic catches and spring-buffered rodstop.

**MIRROR:** First quality ¼" float glass triple-silvered, electro-copper plated with baked enamel backing, guaranteed for 15 years against silver spoilage. Protected by shock-absorbing filler.

**INTERIOR SHELVES:** 22 gauge stainless steel. Four shelves — three adjustable, one fixed. Each shelf area is 60 sq. in.

- ☒ An inherent characteristic of a manufacturing process for tempered glass is distortion which may vary from mirror to mirror.

## Operation

Spring-buffered rodstop prevents door from opening beyond 90 degrees.

## Installation

Verify all rough-in dimensions prior to installation. Recessed unit requires rough wall opening 15<sup>5</sup>/<sub>8</sub>"W x 29<sup>1</sup>/<sub>8</sub>"H x 4"D. Secure to framing with mounting screws (included) at holes provided. Shim at screw points as required. Cabinet may be inverted for left hand door swing.

## Guide Specification

Recessed medicine cabinet consisting of mirror and storage cabinet with four shelves shall be fabricated of stainless steel with exposed surfaces in satin finish. Mirrored door with full-length piano hinge. Interior of storage cabinet to have four shelves — three adjustable and one fixed. Adjustable for right or left hand door swing.

**Overall dimensions: 17<sup>1</sup>/<sub>8</sub>"W x 30<sup>3</sup>/<sub>8</sub>"H x 4"D.**



## ADA Compliant

- ☒ Consult local and national accessibility codes for proper installation guidelines.
- ☒ Conformity and compliance to local and national codes is the responsibility of the installer.

Orders composed of products indicated as **BradEX**® will be available to ship in three days after receipt of order at the factory. There is no pricing penalty for this service from Bradley.

Page 1 of 2

1/24/2024

[View Latest Version](#)

This information is subject to change without notice.

Bradley\_MedicineCabinet\_175\_10\_11

© 2024 Bradley

P.O. Box 309, Menomonee Falls, WI 53052-0309

800 BRADLEY (800 272 3539)

+1 262 251 6000

bradleycorp.com




A WATTS Brand

175

Medicine Cabinet

## Dimensions

(mm)

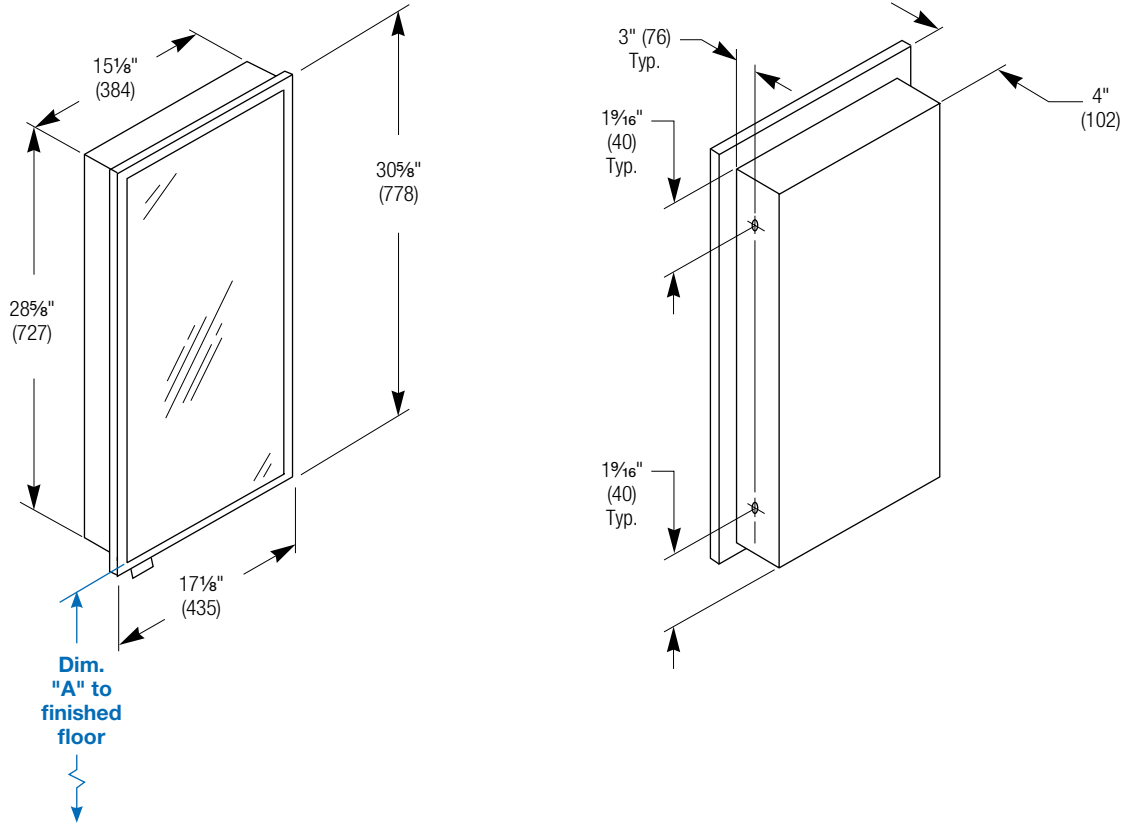

Dim. "A" Key Surface:	For Dim. "A"	Top of Rough Wall Opening	Bottom of Rough Wall Opening
Mirror's bottom edge of the reflecting surface to finished floor	48" (1219)	77 1/4" (1962)	48 1/8" (1222)
	45" (1143)	74 1/4" (1886)	45 1/8" (1146)
	42" (1067)	71 1/4" (1810)	42 1/8" (1070)
	40" (1016)	69 1/4" (1759)	40 1/8" (1019)
<b>Rough wall opening:</b>			
Surface Mount:	No rough opening, see overall dimensions		
Recessed:	15 5/8" (397) Wide x 29 1/8" (740) High x 4" (102) Deep		
Semi-Recessed:	15 5/8" (397) Wide x 29 1/8" (740) High x 2" (51) Deep		

Orders composed of products indicated as **BradEX**® will be available to ship in three days after receipt of order at the factory. There is no pricing penalty for this service from Bradley.

Page 2 of 2

1/24/2024

[View Latest Version](#)

This information is subject to change without notice.

Bradley\_MedicineCabinet\_175\_10\_11

© 2024 Bradley  
P.O. Box 309, Menomonee Falls, WI 53052-0309  
800 BRADLEY (800 272 3539) +1 262 251 6000  
bradleycorp.com